

October 13, 2020


To: Hospitals and Surgeons

Subject: **URGENT MEDICAL DEVICE FIELD SAFETY NOTICE – REMOVAL**

Reference: ZFA 2020-00165

Affected Product: Regenerex® Primary Taper Cap

Item Number: 141269	Description: REGENEREX PRIMARY TAPER CAP	
Lot Numbers:		
015800	324440	685300
023900	324440R	696280
058930	389060	821980
200720	418430	890320
313260	646040	997610

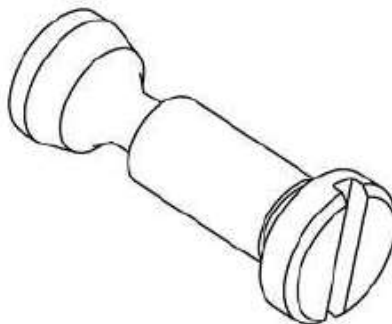

As a precautionary measure Biomet Orthopedics LLC is conducting a lot specific medical device Field Safety Corrective Action (removal) of certain Regenerex Primary Taper Caps, because the above listed item and lot combinations have not been properly aligned with the designated gamma sterilization group. This could result in the product not being properly sterilized. To date no adverse events are reported which could be linked to this issue.

Risks		
Describe immediate health consequences (injuries or illness) that may result from use of or exposure to the product issue.	Most Probable	Highest Severity
	No patient, user, or other stakeholder harm	No patient, user, or other stakeholder harm
Describe long range health consequences (injuries or illness) that may result from use of or exposure to the product issue.	Most Probable	Highest Severity
	No patient, user, or other stakeholder harm	Surgical intervention due to infection

Our records indicate that you may have received one or more of the affected products. The affected units were distributed between January 2011 and October 2019. (Local deployment may differ).

Hospital Responsibilities:

1. Review this Field Safety Notice and ensure that all involved personnel are aware of the contents.
2. If you have affected product at your facility, assist your Zimmer Biomet sales representative and quarantine all affected products. Your Zimmer Biomet sales representative will remove the affected product from your facility.
3. Complete **Attachment 1 – Certificate of Acknowledgement** and send to fieldaction.ch@zimmerbiomet.com. This form will be returned even if you do not have affected products at your facility.
4. Retain a copy of the acknowledgement form with your Field Safety Corrective Action records in the event of a compliance audit of your facility's documentation.
5. If you have further questions or concerns after reviewing this Field Safety Notice, please contact your Zimmer Biomet representative.

Surgeon Responsibilities:

1. Review this Field Safety Notice for awareness of the contents.
2. There are no specific patient monitoring instructions related to this Field Safety Notice that are recommended beyond your existing follow-up schedule.
3. Complete **Attachment 1 – Certificate of Acknowledgement** and send to fieldaction.ch@zimmerbiomet.com. This form must be returned even if you do not have affected products at your facility.
4. Retain a copy of the acknowledgement form with your Field Safety Corrective Action records in the event of a compliance audit of your facility's documentation.
5. If you have further questions or concerns after reviewing this Field Safety Notice, please contact your Zimmer Biomet representative.

Other Information

This medical device Field Safety Notice was reported to all relevant Competent Authorities and the related Notified Body as required under the applicable regulations for Medical Devices as per MEDDEV 2.12-1 in Europe.

Please keep Zimmer Biomet informed of any adverse events associated with this units or any other Zimmer Biomet product by emailing per.ch@zimmerbiomet.com or to your local Zimmer Biomet contact.

Please be aware that the names of user facilities notified are routinely provided to the Competent Authorities for audit purposes.

The undersigned confirms that this notice has been delivered to the appropriate Regulatory Agencies.

We would like to thank you for your co-operation in advance and regret any inconveniences caused by this Field Safety Corrective Action.

Sincerely,



Kevin Escapule
Director, Post Market Surveillance

ATTACHMENT 1
Certificate of Acknowledgement

IMMEDIATE RESPONSE REQUIRED – TIME SENSITIVE ACTION NEEDED

Affected Product: Regenerex® Primary Taper Cap

Field Safety Corrective Action Reference: ZFA 2020-00165

Please return the **completed** form to your Zimmer Biomet contact person or by e-mail

fieldaction.ch@zimmerbiomet.com

I received and understood the Field Safety Notice.

Regarding the parts:

All inventories for the affected products have been checked and following parts are to be returned:

Item Reference	Lot Number	Number of parts returned

OR

The affected products which are unavailable for return have been:

discarded lost other: _____

By signing below, I acknowledge that the required actions have been taken in accordance with the Field Safety Notice.

[] **Hospital Facility** [] **Surgeon** *(Please check one as applicable)*

Printed Name: _____ **Signature:** _____

Date: ____/____/____

Title: _____

Telephone: () ____ - ____

Facility Name: _____

Facility Address: _____

City: _____ **ZIP:** _____

Country: _____